


## DeRoyal<sup>®</sup> SHOULDER PAD III – ABDUCTION DEVICE

Single Patient Use Only  
Rx Only

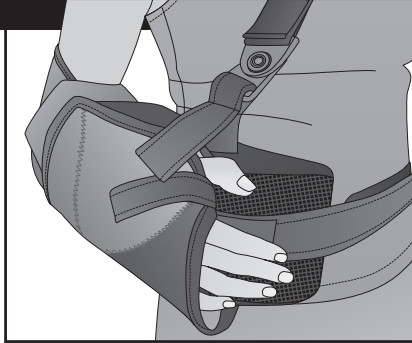

### IMPORTANT INFORMATION

Please read all instructions, warnings and precautions before use. Correct application is essential for proper functioning of product. Use only on the person it was provided to by a healthcare professional and only for the use it was intended.

### INTENDED USE


The DeRoyal<sup>®</sup> Shoulder Pad III is for surgical rotator cuff repairs, anterior glenohumeral capsular reconstruction, dislocation/subluxation of G-H joint, S/P glenohumeral acromioplasty, Bankart repairs, soft tissue repairs, and shoulder sprains and strains.

### PRECAUTIONS


This product is to be fitted by a physician (or properly licensed practitioner) who is familiar with the purpose for which it is intended. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare practitioners or healthcare providers involved in the patient's care as well as the patient. Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

### INSTRUCTIONS FOR USE


1. Brace is initially configured to fit the patient's right shoulder. To configure for the left shoulder, release both




2. Release the front buckle clasp on the shoulder strap where the strap attaches to forearm cuff on sling. **NOTE:** Ensure the front shoulder strap is not twisted before reattaching the buckles.






3. Remove the thumb and forearm straps to completely open the sling.



4. Place affected arm in sling so it rests comfortably in the fold of the sling. Ensure patient's elbow is seated as far back in the fold pocket of the sling as possible. The sling should extend to the first joint of the pinky finger. **NOTE:** Ensure all open wounds are covered before applying device.




5. Sling length can be adjusted by removing the forearm cuff and securing in desired position. **Note:** Attach forearm cuff towards elbow pocket to make sling shorter and



## DeRoyal<sup>®</sup> SHOULDER PAD III – ABDUCTION DEVICE

Single Patient Use Only  
Rx Only

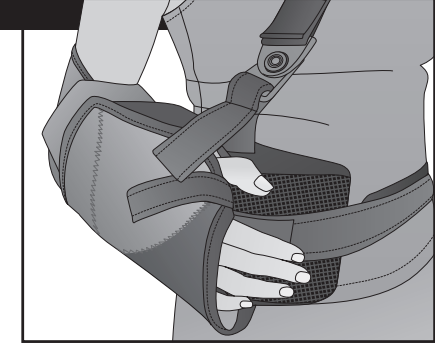

### IMPORTANT INFORMATION

Please read all instructions, warnings and precautions before use. Correct application is essential for proper functioning of product. Use only on the person it was provided to by a healthcare professional and only for the use it was intended.

### INTENDED USE


The DeRoyal<sup>®</sup> Shoulder Pad III is for surgical rotator cuff repairs, anterior glenohumeral capsular reconstruction, dislocation/subluxation of G-H joint, S/P glenohumeral acromioplasty, Bankart repairs, soft tissue repairs, and shoulder sprains and strains.

### PRECAUTIONS


This product is to be fitted by a physician (or properly licensed practitioner) who is familiar with the purpose for which it is intended. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare practitioners or healthcare providers involved in the patient's care as well as the patient. Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

### INSTRUCTIONS FOR USE


1. Brace is initially configured to fit the patient's right shoulder. To configure for the left shoulder, release both




2. Release the front buckle clasp on the shoulder strap where the strap attaches to forearm cuff on sling. **NOTE:** Ensure the front shoulder strap is not twisted before reattaching the buckles.






3. Remove the thumb and forearm straps to completely open the sling.



4. Place affected arm in sling so it rests comfortably in the fold of the sling. Ensure patient's elbow is seated as far back in the fold pocket of the sling as possible. The sling should extend to the first joint of the pinky finger. **NOTE:** Ensure all open wounds are covered before applying device.












5. Sling length can be adjusted by removing the forearm cuff and securing in desired position. **Note:** Attach forearm cuff towards elbow pocket to make sling shorter and



away from elbow pocket to make longer.

6. Reattach the front buckle on the shoulder strap to the receiving buckle attachment located on the forearm cuff of the sling. Reattach the forearm and thumb straps on sling. Note: If desired, rest thumb on adjustable thumb strap for additional comfort.
7. Shoulder strap length can be adjusted at both ends of the strap. To adjust the front of the shoulder strap, remove Y-tab, trim strap to desired length and reapply Y-tab. To adjust the back of the shoulder strap, simple release hook strap and reattach at desired length. NOTE: Shoulder pad should be positioned evenly over non-affected shoulder for comfort.
8. Align the foam block at waistline on patient's affected side. Attach arm sling to the foam block by securing hook and loop portions together.
9. Detach the buckle at end of the foam block. Place waist strap around patient's waist and fasten buckle. To adjust strap length, pull the waist strap for a secure fit. Attach Y-tab hook end back onto strap. Note: If strap is too long, remove Y-tab and trim strap to desired length. The position of the foam block may be adjusted by sliding the block forward or backward along the waistline to



achieve the desired external or internal rotation. If foam block can be pushed downward with pressure, the waist strap should be tightened. Stress ball included to promote proper circulation and encourage exercise.

#### CARE INSTRUCTIONS

Hand wash arm sling and foam block cover in lukewarm water and air dry.

#### WARRANTY

DEROYAL PRODUCTS ARE WARRANTED FOR NINETY (90) DAYS FROM THE DATE OF SHIPMENT FROM DEROYAL AS TO PRODUCT QUALITY AND WORKMANSHIP. DEROYAL'S WRITTEN WARRANTIES ARE GIVEN IN LIEU OF ANY IMPLIED WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.












Scan code for more product information or visit <http://www.deroyal.com/videos/shoulderpadiii>

DeRoyal®  
Improving Care. Improving Business.

Manufactured by DeRoyal Industries, Inc.

©2012 DeRoyal Industries, Inc. All Rights Reserved.  
Part#0-1864 Revised 1/13

1. away from elbow pocket to make longer.
2. Reattach the front buckle on the shoulder strap to the receiving buckle attachment located on the forearm cuff of the sling. Reattach the forearm and thumb straps on sling. Note: If desired, rest thumb on adjustable thumb strap for additional comfort.
3. Shoulder strap length can be adjusted at both ends of the strap. To adjust the front of the shoulder strap, remove Y-tab, trim strap to desired length and reapply Y-tab. To adjust the back of the shoulder strap, simple release hook strap and reattach at desired length. NOTE: Shoulder pad should be positioned evenly over non-affected shoulder for comfort.
4. Align the foam block at waistline on patient's affected side. Attach arm sling to the foam block by securing hook and loop portions together.
5. Detach the buckle at end of the foam block. Place waist strap around patient's waist and fasten buckle. To adjust strap length, pull the waist strap for a secure fit. Attach Y-tab hook end back onto strap. Note: If strap is too long, remove Y-tab and trim strap to desired length. The position of the foam block may be adjusted by sliding the block forward or backward along the waistline to



achieve the desired external or internal rotation. If foam block can be pushed downward with pressure, the waist strap should be tightened. Stress ball included to promote proper circulation and encourage exercise.

#### CARE INSTRUCTIONS

Hand wash arm sling and foam block cover in lukewarm water and air dry.

#### WARRANTY

DEROYAL PRODUCTS ARE WARRANTED FOR NINETY (90) DAYS FROM THE DATE OF SHIPMENT FROM DEROYAL AS TO PRODUCT QUALITY AND WORKMANSHIP. DEROYAL'S WRITTEN WARRANTIES ARE GIVEN IN LIEU OF ANY IMPLIED WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.



Scan code for more product information or visit <http://www.deroyal.com/videos/shoulderpadiii>

DeRoyal®  
Improving Care. Improving Business.

Manufactured by DeRoyal Industries, Inc.  
200 DeBusk Lane  
Powell, TN 37849 U.S.A.  
888.938.7828  
865.938.7828

©2012 DeRoyal Industries, Inc. All Rights Reserved.  
Part#0-1864 Revised 1/13