



Pelvic Support Belt

INSTALLATION AND USER'S INSTRUCTIONS

ART NOS. GB2, HB2, HB4, LB2, LB4, & NB2

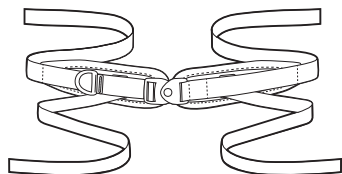

These instructions provide important information for the safe use and maintenance of all Bodypoint pelvic support belts. Give these instructions to the user or their caregiver and review them to ensure that they are understood.

⚠️ WARNING! Product should be installed and fitted by a qualified rehab technician.

For installation, this product should be mounted with one of the following:

- Flat-Mount end-fittings
- Cinch-Mount end-fittings
- Cam buckles (1" suitable for users up to 75kg, 1-1/2" and 2" suitable for all users)

Optional Bodypoint belt mounting hardware may also be used for mounting to wheelchairs and seating systems.

INTENDED USE:

⚠️ WARNING! This product should only be used for positioning a person in a wheelchair or work chair. It is NOT intended for use as a transportation safety device, as a personal restraint device, or in any other application where its failure could result in injury. Misuse of this product is unauthorized and unsafe.

⚠️ WARNING! This pelvic support belt must be worn tightly fitted across the pelvis or thighs at all times. Have your seating specialist demonstrate its proper adjustment and use.

- A loose belt can allow the user to slip down and create a risk of strangulation.
- Accidental release of this pelvic support belt can allow the user to slip down or fall from the wheelchair.
- A user's inability to self-release can be hazardous if the user slips down or is trapped in the chair in an emergency.

If the user's physical or cognitive abilities prevent them from safely operating this belt, a caregiver must be present at all times during its use. Ensure that all caregivers know how to correctly tighten and unfasten the product.

⚠️ WARNING! As with any new seating support, this product may change the way a person sits. Users

must continue to practice regular pressure relief activities and skin integrity checks, not only where this product contacts the user, but also in primary pressure-bearing areas such as the sacrum, legs, and buttocks. If increased skin redness or irritation occurs, discontinue use and consult your physician or seating specialist. Failure to do so may result in serious injury, such as pressure ulcers.

⚠️ WARNING! If a serious incident occurs related to the use of this product, it should be reported to the manufacturer (Bodypoint, Inc.) and the local Competent Authority.

PERIODIC SAFETY AND PERFORMANCE CHECKS:


To ensure user safety, this product must be checked periodically for function and signs of wear. If the product does not function correctly or if significant wear is found in the buckles, mounting points, webbing, padding, or stitches, stop using it and contact your supplier for qualified repair or replacement by Bodypoint. Under no circumstance should this product be altered or repaired by unqualified persons — health and safety depend on it!



CLEANING: Machine wash, hot, 60°C (140°F). Do not bleach. Tumble dry, low temperature, or drip dry. Do not iron. (Placing the product inside a cloth bag during washing helps prevent scratches to the product and the machine.)



SCRAP/DISPOSAL: Product is made of materials which can be disposed of safely without special precautions at the end of its useful life.

WARRANTY: This product carries a limited lifetime warranty against defects in workmanship and materials arising under normal use by the original consumer. Contact your supplier or Bodypoint for warranty claims.

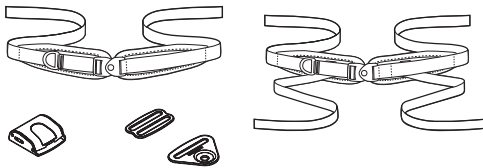



PACKAGE CONTENTS

- Two-Point or Four-Point Pelvic Support Belt
- Set of Cinch-Mount™ or Flat-Mount™ End-Fittings (Optional)
- FrameSaver™ Clamps (Optional)




INSTALLATION: TWO-POINT PELVIC SUPPORT BELTS

1. Based on clinical goals, determine the most effective position and angle for the belt. Determine whether putting pull strap on left or right side is best for user.
2. Locate desired mounting points on the seating system or wheelchair frame.
3. Attach end-fittings to rigid seat base or wheelchair frame using optional Bodypoint belt mounting hardware, if needed.
4. Center the belt on the user, thread the strap ends through the end-fittings, and adjust to desired length.
5. Tighten the belt until it is snug.



INSTALLATION: FOUR-POINT PELVIC SUPPORT BELTS

1. Follow the installation instructions above to fit and install the belt to stabilize and position the user.
2. Attach the secondary straps to the wheelchair to prevent the belt from shifting.

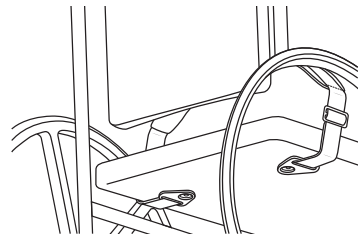

DIRECT MOUNTING OPTION


End-fittings can be attached directly to solid seat surfaces. Mounting screws must have minimum pullout strength of 90kg/200lbs. (Not included in package.)



ADJUSTMENT

When the belt is properly adjusted and tightened, it should fit snug, with all slack removed, so that the user is secure.

Use the pull strap for daily adjustments, such as to accommodate changes in clothing. If additional length adjustment is necessary to achieve a good fit or the belt needs to be removed for cleaning, this can be done using the belt end-fittings.



SAFETY CHECK

When properly positioned in wheelchair, have user lean forward and side to side to check fit. Check for:

1. Normal operation of buckle and adjustment straps.
2. Comfort – Look for areas of irritation.
3. Position – If too high or too low, adjust mounting points.
4. Move chair through full range of motion, including tilt, folding, and rolling. Check for any interference and relocate mounting points as necessary.