


Universal Elastic Strap

INSTALLATION AND USER'S INSTRUCTIONS

ART NOS. SP110S, SP110L, SP110XL, SP111S, SP111L & SP111XL

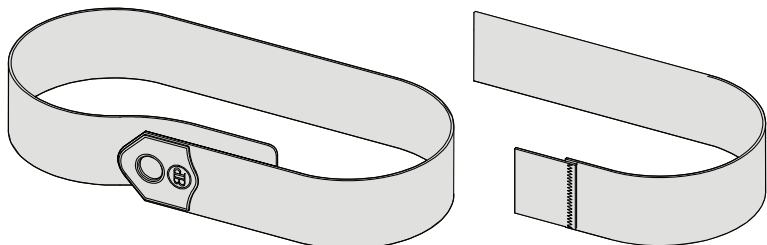

These instructions provide important information for the safe use and maintenance of all Bodypoint Universal Elastic Straps. Give these instructions to the user or their caregiver and review them to ensure that they are understood.

⚠ WARNING! Product should be installed and fitted by a qualified rehab technician.

⚠ WARNING! Because of the risk of choking, it is dangerous to use this product without stabilizing the pelvis – always use with a properly fitted pelvic support belt.

INTENDED USE:

⚠ WARNING! This product should only be used for positioning a person in a wheelchair or work chair. It is NOT intended for use as a transportation safety device, as a personal restraint device, or in any other application where its failure could result in injury. Misuse of this product is unauthorized and unsafe.

⚠ WARNING! This positioning belt must be properly fitted to support the user's body without causing injury. Have your seating specialist demonstrate its proper adjustment and use.

- If it is too tight across the shoulders and chest, it can restrict respiration and increase pressure.
- If it is too loose, it can allow the user to slip down and may create a risk of strangulation.
- Accidental release of this product can allow the user to fall forward or fall from the wheelchair.
- A user's inability to self-release can be hazardous if the user slips down or is trapped in the wheelchair in an emergency.

If the user's physical or cognitive abilities could prevent them from safely operating this product, a caregiver must be present at all times during its use. Ensure that all caregivers know how to correctly adjust and unfasten the product.

⚠ WARNING! As with any new seating support, this product may change the way a person sits. Users must continue to practice regular pressure relief activities and skin integrity checks, not only where this product contacts the user, but also in primary

pressure-bearing areas such as the sacrum, legs, and buttocks. If increased skin redness or irritation occurs, discontinue use and consult your physician or seating specialist. Failure to do so may result in serious injury, such as pressure ulcers.

⚠ WARNING! If a serious incident occurs related to the use of this product, it should be reported to the manufacturer (Bodypoint, Inc.) and the local Competent Authority.

PERIODIC SAFETY AND PERFORMANCE


CHECKS: To ensure user safety, this product must be checked periodically for function and signs of wear. If the product does not function correctly or if significant wear is found in the buckles, mounting points, webbing, padding, or stitches, stop using it and contact your supplier for qualified repair or replacement by Bodypoint. Under no circumstance should this product be altered or repaired by unqualified persons — health and safety depend on it!



CLEANING: Machine wash, hot, 60°C (140°F). Do not bleach. Tumble dry, low temperature, or drip dry. Do not iron. (Placing the product inside a cloth bag during washing helps prevent scratches to the product and the machine.)

SCRAP/DISPOSAL: Product is made of materials which can be disposed of safely without special precautions at the end of its useful life.


WARRANTY: This product carries a limited-lifetime warranty against defects in workmanship and materials arising under normal use by the original consumer. Contact your supplier or Bodypoint for warranty claims.

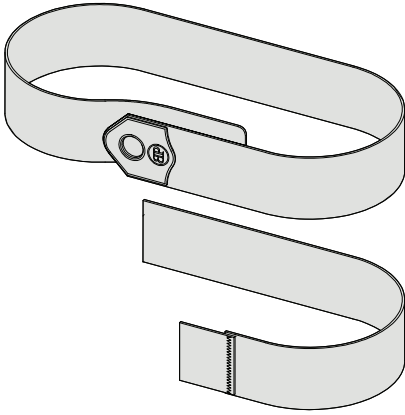


PACKAGE CONTENTS

Package may contain one or more of the following:


- Universal Elastic Strap
- Elastic Extension Strap



To make shorter, cut to length.

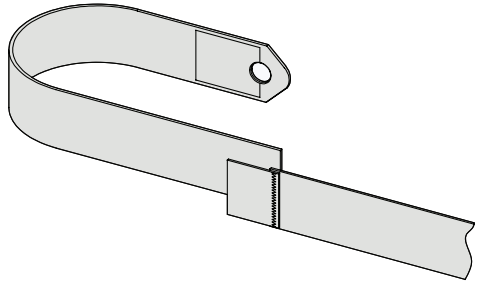

To make longer, add Elastic Extension Strap.

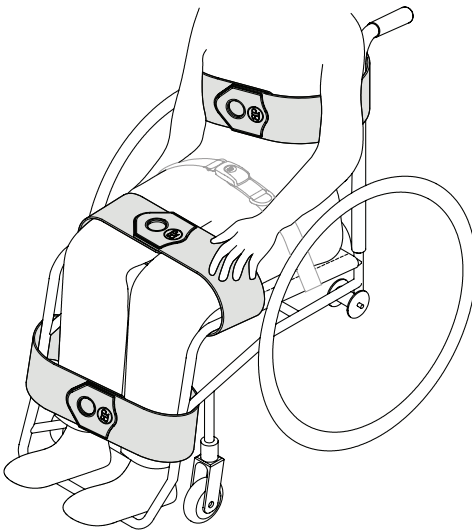

POSITIONING

Universal Elastic Straps provide temporary positioning support, and can be placed in multiple locations to suit the user's needs. For long-term positioning solutions consider more individualized products offered by Bodypoint.

SAFETY CHECK

When properly positioned in wheelchair, have user lean forward and side to side to check fit. Check for:

1. Comfort – If any rubbing occurs relocate straps.
2. Position - If too high or too low, adjust location.
3. Interference with other devices – Relocate straps as necessary to clear armrests, accessory pads, or feeding tubes.
4. Move chair through full range of motion, including tilt, folding, and rolling. Check for any interference.