

Pacer Gait Trainer

K620, K630, K640 & K650 Product Manual




Contents


Important information	3
Safety messages	4
Recommended use User and item dimensions	5
Check your order and basic components	6
Upper frames	
Standard and dynamic	7
Base frames	
Standard, utility and treadmill/stability	8
Casters and wheels	9
Accessories	
Odometer and clamps	10
Hand loops	11-12
Arm prompts/arm platforms	13-15
Handbrake	16
Chest prompt	17
Hip positioner	18
Hip positioner pad	19
Pelvic support	20-21
Thigh prompts	22
Ankle prompts	23
Tray	24
Multi-position saddle	25
Guide bar	26
Operation	27-29
Maintenance, cleaning, and warranty	30
Materials and user modifications	31

Key for users

Use this key to determine which sections of this product manual apply to you.

 **Technical Users** For professionals who order and set up Rifton products.

 **Home Users** For care-givers who use Rifton products on a regular basis.

 **Maintenance Personnel** For anyone who is responsible for service or re-ordering of Rifton products and parts.

WARNING




- Thoroughly read and understand the information in this product manual before attempting to use this product. If the procedures and instructions in this product manual are not followed, serious injury or death could occur.
- A qualified professional must assess the appropriateness and safety of all equipment for each client.
- This product is intended for use by clients of unreliable judgment. Adult supervision is required at all times.
- To prevent falls and injuries:
 - Do not use this product on rough and uneven terrain, around swimming pools or near stairways.
 - Ensure the appropriate use of straps and supports at all times. Straps and supports are provided for the safety of the user and must be carefully adjusted for comfort and security.
 - Tighten all adjustment knobs before use and immediately after making any adjustments.
 - Position accessories so that the client's weight is centered between the casters.
- Do not use this product for clients outside the height and weight limits specified in this manual.
- To prevent structural failure, which may result in serious injury or death:
 - Inspect this product and accessories regularly for loose or missing screws, metal fatigue, cracks, broken welds, missing attachments, general instability or other signs of excessive wear.
 - Immediately remove this product from use when any condition develops that might make operation unsafe.
 - Do not use Rifton components or products for any purpose other than their intended use.
- Adequately supervise use of the Pacer to prevent:
 - Excessive movement and speed
 - Sudden stops from hitting a curb, cracks, or debris
- Use adequate accessories to ensure that user's feet remain within boundaries of the Pacer frame.
- Use special care and supervision when using the Pacer under conditions which might affect stability, including:
 - Uneven ground
 - Ramps, slopes or hills
 - Clients who experience strong involuntary movements or seizures

Recommended use

The Pacer gait trainer is a Class 1 medical device. It is designed to help a client learn to walk. For a client lacking active use of his or her trunk and leg muscles, the Pacer provides the necessary support during gait training and requires little or no weight-bearing.

User and item dimensions

User dimensions – inches (cm)		K620 small	K630 med	K640 large	K650 XL
Elbow height		18½-27½ (47-70)	24-35 (61-89)	32-47 (81-119)	34-49 (86-124)
	Key user dimension: elbow height Measure the vertical distance from the bent elbow to the floor while the user is standing upright. Choose the gait trainer that allows for growth.				
	Important: Make sure that the chest prompt width is adequate, allowing for growth. User's weight must not exceed the maximum working load.				

Item dimensions – inches (cm)		K620 small	K630 med	K640 large	K650 XL
Floor to top of arm prompt		18½-27½ (47-70)	24-35 (61-89)	32-47 (81-119)	34-49 (86-124)
Overall width	Standard base:	23 (58)	26 (66)	28 (71)	31½ (80)
	Utility base:	N/A	30 (76)	32 (81)	N/A
	Narrow treadmill base:	35 (89)	35 (89)	35 (89)	N/A
	Wide treadmill base:	40 (102)	40 (102)	40 (102)	N/A
Overall length	Standard base:	26 (66)	30 (76)	36 (91)	39¾ (101)
	Utility base:	N/A	36 (91)	40½ (103)	N/A
	Treadmill bases:	41 (104)	41 (104)	41 (104)	N/A
Frame height	Standard & utility bases:	16-21 (41-53)	21½-27 (55-69)	28½-38½ (72-98)	31-41 (79-104)
	Treadmill bases:	23-35 (58-89)	23½-36½ (60-93)	30-47 (76-119)	N/A
Base height (without upper frame)	Standard & utility bases:	11 (28)	14½ (37)	16 (41)	18½ (47)
	Treadmill bases:	21 (53)	21 (53)	21 (53)	N/A
Frame weight - lbs. (kg)	Standard base:	11½ (5.2)	15 (6.8)	15½ (7)	22½ (10.2)
	Utility base:	N/A	18½ (8.4)	19¼ (8.7)	N/A
	Narrow treadmill base:	27½ (12.5)	27½ (12.5)	27½ (12.5)	N/A
	Wide treadmill base:	28 (12.7)	28 (12.7)	28 (12.7)	N/A
	Standard upper:	6 (2.7)	7½ (3.4)	9½ (4.4)	11 (4.9)
Dynamic upper movement	Dynamic upper:	7½ (3.4)	11½ (5.2)	13½ (6.1)	15 (6.8)
	Vertical:	1¼ (3.5)	2 (5)	2 (5)	2 (5)
Max. treadmill width	Horizontal:	1½ (4)	2 (5)	2 (5)	2 (5)
	Narrow treadmill base:	29 (74)	29 (74)	29 (74)	N/A
Max. treadmill height	Wide treadmill base:	34 (86)	34 (86)	34 (86)	N/A
	Treadmill bases:	11 (28)	11 (28)	11 (28)	N/A
Max. working load-lbs. (kg)		75 (34)	150 (68)	200 (91)	250 (113)

Check your order

The Pacer frame and accessories that you specified in your order may be shipped in more than one carton. Use the diagrams in this manual to make sure your order is complete.

If your shipment is incomplete or in any way damaged on arrival, please call Customer Service.

Basic item

⚠ CAUTION Ensure that column is fully inserted and latched into base frame prior to using Pacer.

Any upper frame can be attached to any base of the same size. Additionally, any medium upper frame may be attached to any large base, increasing the height range of the medium by 1" (3 cm). The large upper frame cannot be used with a medium base.

Figure 6a: To attach the upper frame to the base, slide the column into the base frame, as shown. To detach the upper and lower frames, press button (A) and slide column out of base frame.

The upper frame and base can be detached for storage or transport.



Figure 6a

Upper frames

Height adjustment

Figure 7a: To adjust the frame up or down, use use trigger (A).

Standard upper

The standard upper frame adjusts in height and provides support for various prompts and accessories.

Dynamic upper

CAUTION To prevent serious injury:

- Keep hands clear of dynamic body support mechanism while Pacer is in use.
- When dynamic weight-bearing and/or lateral weight shift mechanisms are unlocked, position arm prompts so that client's hands are kept clear of frame and column.

Figure 7b: The dynamic upper provides dynamic body support by allowing up/down and side-to-side movement of the upper frame.

To lock or unlock vertical up/down movement (dynamic weight-bearing), lift upper frame to unweight system and use trigger (B).

To lock or unlock side-to-side movement (dynamic weight-shift), use trigger (C).

Medium, large and XL only:

The default force range of the dynamic weight bearing system will be fine for most users. However, it can be adjusted if needed, by turning screw (D) with a 3/16" hex wrench. Turning the screw clockwise increases force.

NOTICE To avoid damaging the DWB system, stop turning when the screw bottoms out (maximum force) or when the screw becomes loose (minimum force).

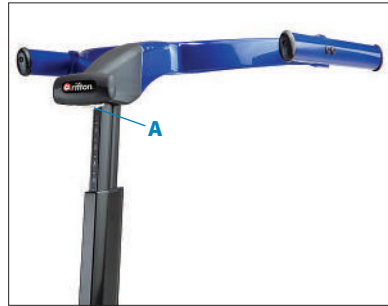


Figure 7a

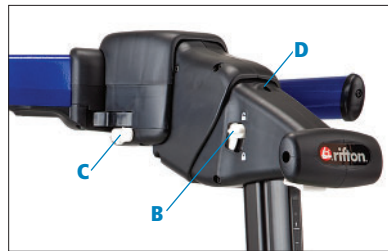


Figure 7b

Base frames

Standard base

Figure 8a: The standard base has four 5½" casters (4" for the small). Each caster has a brake, drag, swivel lock and directional lock. An odometer is an optional accessory.



Figure 8a

Utility base

Figure 8b: The utility base has two 8" front casters and two 11½" rear wheels. Directional lock, brake and drag functions are provided by the rear wheels. Swivel lock is provided by the front casters. An odometer is an optional accessory.



Figure 8b

Treadmill/stability base

▲ WARNING To prevent serious injury or death:

- Do not position client facing the open end of Pacer frame when on the treadmill.
- Stop treadmill before making adjustments.
- Keep extremities clear of adjustment mechanism.

▲ CAUTION To prevent serious injury:

- Always lock caster brakes when Pacer is over the treadmill.
- Always use pelvic support, hip positioner or multi-position saddle when client is on the treadmill.
- Do not run treadmill in reverse when using Pacer.

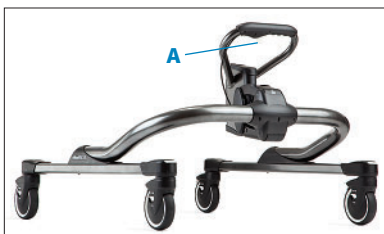


Figure 8c

Figure 8c: The treadmill/stability base is a wide, height adjustable base frame designed for use both overland and over a treadmill. It can be used with the large, medium and small upper frames.

Use trigger (A) to adjust frame downward for overland use, or upward as necessary to provide clearance over a treadmill.

Tip: This base is available in two widths, standard and wide. See dimension chart on page 5 for sizing.

Casters/wheels

Adjustments

Figure 9a:

The **Swivel lock** prevents the caster from swiveling.

- To **engage the swivel lock**: press button (A).
- To **disengage**, press button (B).

Locking all four casters will keep the client traveling in a straight line.

Locking the rear casters (those behind the client) will help stabilize the client, while still allowing for turning.

To **engage caster brake** (C), press lower part of brake pedal. To release the brake, press upper part of brake pedal.

To **engage the wheel brake** (utility base), press brake pedal (D). To release the wheel brake, lift brake pedal (E).

To **engage caster drag** (standard base) or wheel drag (utility base), rotate dial (F).

Directional lock (F) allows the caster or wheel to turn in one direction only, helpful for clients who may involuntarily roll backward while trying to walk. To engage the directional lock:

- Push lever (F) down until it snaps into place.
- When the directional lock is engaged, the caster or wheel will make a clicking noise while moving forward and lock when pushed backward.



Figure 9a

Accessories

Odometer

Figure 10a: The odometer displays distance traveled. To reset display to 0, press button (A). To display total lifetime distance traveled, press and hold button (A) for one second. Lifetime distance will be displayed in kilometers or thousands of feet, depending on unit setting.

To switch between feet or meters, press and hold button (A) until units change (approximately 10 seconds).



Figure 10a

Clamps

Attaching and removing

Figure 10b: Most accessories are attached to and removed from the frame with clamps (B) and posts (C).

1. Loosen knob (D) and swing it down.
2. Swing band (E) up.
3. Place clamp (B) around oval bar.
4. Swing knob (D) up into slot on band (E).
5. Tighten thoroughly.

Placement of accessories on the frame will vary according to the position and abilities of the client and the number of accessories used.

Figure 10c: For slimmer clients, the clamps for any accessory can be attached on the inside of the top bar. This positions accessories closer to the client. To reposition posts (see page 15).

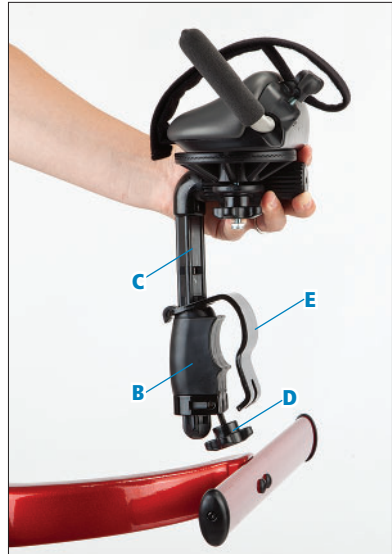


Figure 10b



Figure 10c

Hand loops

⚠️ WARNING

To prevent tipping and resulting injury, do not position handloops, arm prompts or arm platforms at the extreme ends of the top bar (see figure 11a).

Attaching

When the Pacer is used in the anterior position, it is recommended that hand loops are attached forward of the frame cross bar. This creates stable positioning and leaves plenty of room for other accessories.

Figure 11b: Hand loop clamps can be attached on the outside of the top bar.

Figure 11c: For slimmer clients, the clamps for any accessory can be attached on the inside of the top bar. This will position the prompts closer to the client. To reposition the hand loop posts (see page 15).



Figure 11a



Figure 11b



Figure 11c

Adjustments

Figure 12a:

Loosen knob (A) to:

- Completely remove the hand loop and clamp.
- Or slide the hand loop toward or away from the client along the top bar.

To adjust height of hand loop:

- Press button (B) and slide post up or down to desired position.
- Release button (B) and push hand loop to engage post.

To tilt hand loop:

Loosen knob (C) and tilt hand loop to desired position. Tighten knob to secure.

To reposition the entire hand loop:

- Completely remove the hand loop from the Pacer (see figures 10b and 10c). Attach inside or outside the top bar (see figures 13b and 13c).
- Press button (B) and completely remove the post, now rotate the post to the desired position, insert it back into clamp and slide to desired height.



Figure 12a

Arm prompts

⚠️ WARNING

To prevent tipping and resulting injury, do not position handloops, arm prompts or arm platforms at the extreme ends of the top bar (see figure 13a).

Attaching

When Pacer is used in the anterior position, it is recommended that arm prompts are attached forward of the frame cross bar. This creates stable positioning and leaves plenty of room for other accessories.

Figure 13b: The arm prompt clamps can be attached on the outside of the top bar.

Figure 13c: For slimmer clients, the clamps for any accessory can be attached on the inside of the top bar. This positions accessories closer to the client. To reposition clamps and posts (see pages 10 and 15).

Adjustments

Figures 13b and 14a:

Loosen knob (A) to:

- Slide arm pad toward or away from the client along the post.
- Rotate up or down.
- Rotate in or out.
- Move the arm pad backward or forward.

To adjust the height of arm prompt:

1. Press button (B) and slide post to desired position.
2. Release button and push post to engage it.

Or completely remove the arm prompt from the Pacer by pressing button (B) and pulling out the post.



Figure 13a



Figure 13b attached outside top bar



Figure 13c attached inside top bar

To adjust the handgrip:

Figure 14a:

1. Loosen knob (C).
2. Slide handgrip forward or back for different forearm lengths, or rotate the handgrip from side to side. Arm strap (D) and wrist strap (E) secure the client's arm in the arm prompt.

Using the wrist strap prevents the client's arm from inadvertently coming out of the arm prompt.

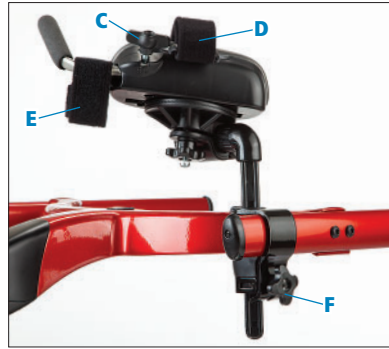


Figure 14a attached inside top bar

To reposition the entire arm prompt:

1. Loosen knob (F).
2. Slide arm prompt to desired position on the top bar of the frame.

Arm platforms

⚠ WARNING To prevent tipping and resulting injury, do not position handloops, arm prompts or arm platforms at the extreme ends of the top bar (see figure 14b).

Attaching see pages 10 and 13.

Adjustments

Figure 14c:

Loosen knob (A) to:

- Slide arm platform toward or away from the client along the post.
- Rotate side to side.
- Rotate 360°.

To adjust the height of arm platform:

1. Press button (B) and slide post to desired position.
2. Release button and push post to engage it.

Or completely remove the arm platform from the Pacer by pressing button (B) and pulling the post out of the clamp.



Figure 14b



Figure 14c



Figure 14d

Figure 15a: Arm straps (C) secure the client's arm in the arm platform. They can be removed completely, if desired. Unfasten the strap and pull it out of the slot beneath the platform.

To reposition the entire arm platform:

1. Loosen knob (D).
2. Slide arm platform to desired position on the top bar of the frame.

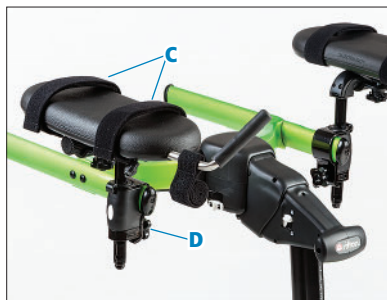


Figure 15a

Figure 15b:

To adjust the optional handgrip:

1. Loosen knob (E).
2. Slide handgrip forward or back for different forearm lengths, or rotate the handgrip from side to side. Arm strap (F) and wrist strap (G) secure the client's arm in the arm platform.

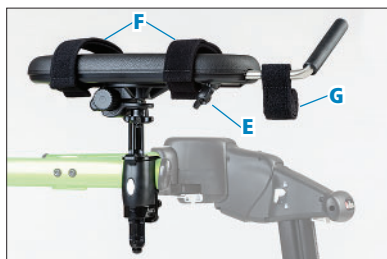


Figure 15b

Post adjustments   

Arm prompt/platform posts can be removed and repositioned to adjust the width between arm prompts/platforms.

Figure 15c and 15d: Clamps can be removed and repositioned to further adjust the width between arm prompts/platforms.

- **Step 1:** Loosen knob (A) and remove arm prompt pad. Figure 15c shows the clamp on the inside of the top bar.
- **Step 2:** Press button (B), lift post out of clamp, and turn to desired position.
- **Step 3:** Insert post back into clamp, slide arm prompt pad back onto post, and use button (B) to adjust the height of the arm prompt. Figure 15d shows the clamp on the outside of the top bar, which increases the width between prompts.

(To remove or attach clamps, see p. 10.)



Figure 15c



Figure 15d

Handbrake

⚠️ WARNING To prevent serious injury or death:

- Use Pacer only on smooth level surfaces.
- Hand brake is not intended to stop Pacer on hills.
- Adult supervision is required at all times.

Attaching to base

Figure 16b:

1. Hook ball at end of cable onto silver clip (A) located inside plastic housing (B) on base.
2. Pull cable housing forward and down to clip into the socket (C) of the plastic housing on base.
3. Clip both brake cables together with the brake cable clip.



Figure 16a

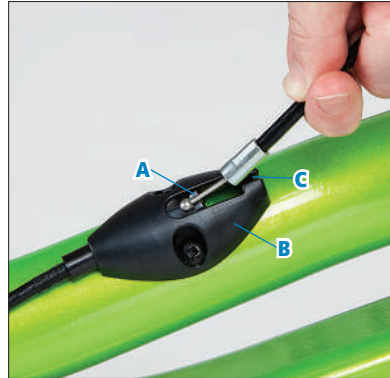


Figure 16b

Detaching from base

Pull cable out of socket (C) in plastic housing (B) on base and lift up. Ball end of cable will pop out of clip (A).

Operation

Figure 16c:

1. Squeeze lever to apply brake.
2. Push lever down (away from handle) to apply parking brake.

Adjustments

Figure 16c: To adjust brake, loosen or tighten knob (D) till desired braking action is reached. A 1/16" gap between rear wheel and brake arm is recommended

See page 13 for arm prompt adjustments.



Figure 16c

Tip (figure 16c): If cable will not pull far enough to clip into the socket of the plastic housing, tighten adjustment knob (D) on brake handle by turning knob clockwise.

Chest prompt

Attaching

⚠️ WARNING To prevent tipping, falls and resulting injury or death:

- Position chest prompt so that the client's center of gravity is centered between the casters.
- Tighten all adjustment knobs on chest prompt prior to use.

Figure 17a: Attach chest prompt directly behind the frame cross bar. The front of the chest prompt has a containment loop to keep the pads together. Rear opens for easy access.

Adjustments

To adjust width of chest prompt:

- Place clamps on the inside or the outside of the top bar (see previous pages).
- Loosen knobs (C) to slide sides of chest prompt in or out.
- Retighten knobs.

To rotate chest prompt:

- Loosen knobs (C) completely.
- Rotate prompt to desired position.
- Retighten knobs.

To adjust height of chest prompt:

- Press buttons (B) and slide posts to desired height.
- Release buttons (B) and push post to engage it.

Reposition or remove entire chest prompt:

- Loosen knobs (A).
- Slide chest prompt backward or forward and retighten knobs (A).
- To remove clamps, see page 10.



Figure 17a

Straps (D) can be adjusted independently to tighten or loosen the chest prompt or to adjust the forward leaning angle of the client. Chest prompt opens front and back. This allows the client to be placed in the anterior or posterior position (see pages 27, 28 and 29).

Hip positioner

Attaching

⚠️ WARNING To prevent tipping and resulting injury, do not position prompts at the rear ends of the top bar (see figure 18a).

Figure 18b: The hip positioner is designed to encourage forward-leaning. Attach this accessory with its two clamps and handholds a few inches away from the end of the top bar. Attach straps with buckles (A) in front of the frame cross bar.

Refer to the warning above for important safety information.

To attach the front of the hip positioner:

- Use buckles (A), attaching them at desired location in front of cross bar.

To attach rear of hip positioner:

- Attach rings (B) to handholds.

Adjustments

To adjust position of handholds on frame:

- Loosen knob (C).
- Slide handholds and clamps to desired position on frame.

To adjust rear height of hip positioner:

- Press button (D) and raise handholds to desired height.
- Release button (D) and push down handholds to engage them.

To raise and lower hip positioner use strap adjusters (E) at back and (F) at front.



Figure 18a

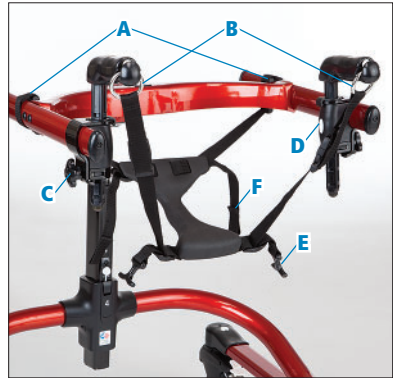


Figure 18b

Hip positioner pad

Assembly

Figure 19b:

1. Push the rear straps of the **hip positioner** through the crossed over straps and pull the **pad** into place.
2. Snap front and side flaps of **pad** together around the **hip positioner**. Make sure both snaps are securely fastened.
3. Attach hip positioner on Pacer.



Figure 19a



Figure 19b Underside of hip positioner with pad

Pelvic support

Attaching

⚠️ WARNING To prevent tipping and resulting injury, do not position prompts at the rear ends of the top bar (see figure 20a).

Figure 20b: The pelvic support provides weight-bearing assist. It is an alternate option to the hip positioner. Attach this accessory with its two clamps and handholds a few inches away from the end of the top bar. Attach straps with buckles (A) in front of the frame cross bar.

Refer to the warning above for important safety information.

To attach front of pelvic support

- Use buckles (A) to attach the pelvic support at the optimal location indicated for positioning. Locations for strap attachment may include any secure position along the top bar of the frame in front of cross bar, at the base of the clamps/accessories in use or at the chest prompt cross bar.

To attach rear of pelvic support

- Attach rings to handholds (B).



Figure 20a

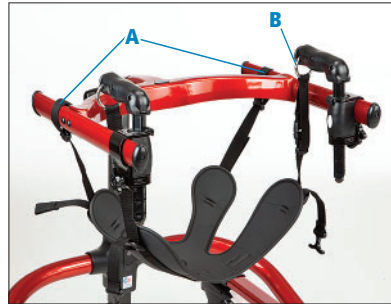


Figure 20b

Adjustment

Figure 21a:

To adjust rear height of pelvic support:

- Press buttons (A) and slide handholds to desired height.
- Release buttons (A) and push down on handholds to engage them.

To adjust position of handholds on frame:

- Loosen knob (B).
- Slide handholds and clamps backward or forward on the frame.

To raise and lower pelvic support:

- Use strap adjusters at front (C) and back (D) of pelvic support.



Figure 21a

Thigh prompts

Attaching

Figure 22a: Thigh prompts work best if attached behind the chest prompt on top bar. Thigh prompt clamps are slightly different from the clamps of other accessories, but attach to the top bar in the same manner (see page 10).

Adjustments

Figure 22b:

1. To swing the thigh pad toward or away from the client:

- Loosen knob (A).
- Adjust thigh pads (B) and re-tighten.

2. To move the thigh pads up or down, or to rotate the thigh pad to a comfortable position against the client's leg:

- Loosen knob (C).
- Adjust thigh pads (B) and re-tighten.

3. To reposition thigh prompts on frame:

- Loosen knob (D).
- Slide clamp along the top bar of the frame.
- Or completely remove the thigh prompts from the Pacer.

4. To secure and adjust strap around the thigh of the client, use buckle adjuster (E).



Figure 22a

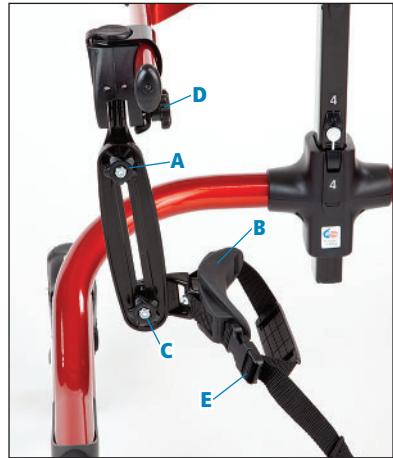


Figure 22b

Ankle prompts

Attaching

Figures 23a – 23c:

- Utility base: insert end of rod opposite latch (A) into rear wheel slot (B). Pull back white latch (A), and release into front slot under frame leg (C).
- Standard base: pull back white latches and release into slots under frame legs.

Adjustments

Figure 23d:

- To secure, loosen or tighten strap around the ankle of the client, use buckle adjuster (D).
- Strap (E) can be adjusted to help guide the stride of the client.
- To limit or increase the stride of the client, squeeze and slide spring adjusters (F) along rods.

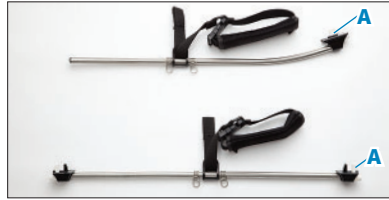


Figure 23a



Figure 23b



Figure 23c

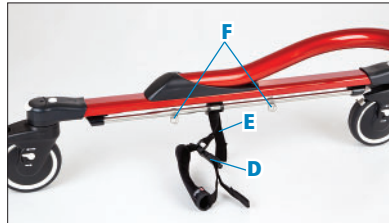


Figure 23d

Tray

⚠️ WARNING To prevent tipping and resulting injury:

- Do not use the tray as a restraint or body support.
- Directly supervise client's use of the tray.
- Do not place more than 10 lb. (4½ kg) on tray.

Attaching

Figure 24a: The tray attaches to the Pacer with a clamp (C) (see page 10 for clamp attachment instructions).



Figure 24a

Adjustments

Figures 24a and 24b:

To reposition tray:

- Loosen knob (A), and swing tray to desired position, then tighten knob.

To adjust angle of tray:

- Loosen knob (B).
- Change the tilt angle of the tray.
- Rotate the tray from side to side, then tighten knob.

To adjust the height of the tray:

- Press button on front of clamp (C).
- Slide post to desired height.
- Release button and push tray up/down to engage post.

To remove insert (D):

- Push fingers up through holes in tray (G).
- Re-install insert (D) by placing tabs (E) in slots (F) and pressing down on front edge of insert until it snaps in place.



Figure 24b

Multi-position saddle

⚠️ WARNING To prevent falling and resulting injury, the hip corral strap should be used for all non-weight-bearing clients, or any time additional security is needed.

Attaching

Medium and large MPS, Figure 25a:

- To attach large saddle under upper frame press button (B) and insert saddle upright into the recess under the cross bar.
- To remove saddle press both button (A) and safety button (B) simultaneously.



Figure 25a

Small MPS, Figure 25b:

- To attach the small saddle under the upper frame push the upright square tube into the recess under the cross bar.
- To remove the small saddle, push the two spring buttons indicated and remove saddle from the recess under the cross bar.



Figure 25b

Adjustments Figure 25c:

- **To adjust height** press trigger (C).
- **To adjust seat angle** press button (D).
- **To adjust seat forward or backward** press trigger (E).
- **To adjust hip corral in or out**, or to attach or remove it, press trigger (F).
- **To remove seat** first remove hip corral, then slide seat using trigger (E) as far back as possible. Finally, press 2 buttons on each side (G) to complete removal.
- **To adjust hip corral height** press trigger (H).
- **To attach corral strap** clip hook onto rear of seat. The corral strap as well as the pads on the hip corral can be removed, if desired. To remove pads, undo hook and loop patch between pads and slide pads off bar. To detach corral strap, remove pads, then press small white buttons near end of bar and pull rings from slots.



Figure 25c

Tip: Every white lever or button indicates a point of adjustment.

Guide bar

▲WARNING To prevent injury, adult supervision is required at all times. Always remove guide bar when not in use.

The guide bar is available for the small, medium and large sizes.

Attaching

1. **Figure 26a:** Attach to either side of the center section on the base frame.
2. **Figure 26b:** The guide bar is attached by swinging the cam lever (A) down to engage the clamp.

Adjustments

1. The guide bar can be rotated to be positioned behind the user or in front.
2. **Figures 26b and 26c:** If the guide bar will not stay in position, adjust it by raising the cam lever (A) up and tighten by turning it clockwise in $\frac{1}{2}$ turn increments. Then swing the cam lever back down.

Note: the lever can be positioned in either direction.



Figure 26a



Figure 26b



Figure 26c

Operation

Once the accessories are attached and adjusted approximately, the client can be placed in the Pacer in either an anterior or posterior position.

⚠ WARNING To prevent tipping and resulting injury:

- Position prompts so that the client's center of gravity is centered between the casters.
- Use adequate accessories to ensure that client's feet remain within boundaries of the Pacer frame.
- Do not position arm prompts, arm platforms or handloops at the extreme ends of the top bar.

Anterior positioning

Forward facing

Figures 27a and 27b: This shows normal positioning. Note that the chest prompt has no tilt and the slightly forward-leaning angle of the client is achieved by locating the hip positioner / pelvic support behind the shoulders.

1. Apply the caster brakes to immobilize the Pacer.
2. Approximate the adjustments of:
 - chest prompt
 - arm prompts
 - hip positioner or pelvic support
 - frame height (top bar of frame).
3. Unfasten:
 - Hip positioner or pelvic support rings at rear of Pacer
 - Buckles at the rear of the chest prompt
 - Straps of arm prompts, thigh prompts and ankle prompts



Figure 27a



Figure 27b

4. Place the client in the Pacer
 - Fasten the rear buckles of the chest prompt.
5. Pull the hip positioner or pelvic support through the legs and:
 - Connect the rings to the handholds or fasten buckles if preferred.
6. Secure the forearms with arm prompt straps.
7. Fasten straps to:
 - Secure the thigh prompt straps around the client's legs.
 - Secure the ankle prompt straps around the client's ankle.
8. Release the caster brakes.

Forward-leaning

Figure 28a: This shows how a more extreme forward-leaning angle is achieved. Note the chest prompt tilt and the location of the hip positioner behind the shoulders. The front hip positioner straps are attached to the chest prompt posts. The arm prompt clamps are attached ahead of the cross bar.

1. To adjust the client's forward-leaning angle:

- Use the chest prompt tilt adjustment (see figures 27a, 27b and 28a).
- Position the top of the chest prompt away from the armpits to avoid pressure and discomfort.

2. Adjust hip positioner or pelvic support:

- Adjust height of handhold posts.
- Use straps to adjust hip positioner or pelvic support angle and to position client's pelvis in the desired forward-leaning angle in relation to the chest prompt (see figures 27a, 27b, 28a).



Figure 28a

3. Adjust arm prompts, arm platforms or hand loops:

- Adjust the width, height and angles of arm prompts (see pp 13–14) or handloops (see page 11).

4. Adjust thigh prompts:

- Adjust the height, angle and strap length to guide the stride of the client (see page 22).
- The thigh prompt is important for positioning the client's thighs closer together or further apart. It also prevents the client's body from twisting in the Pacer.

5. Adjust ankle prompts:

- Adjust straps and spring adjusters to guide the stride of the client (see page 23).

6. Adjust the tray position and angle (see page 24).

7. Release the caster brakes.



Figure 29a

Posterior positioning

Rear facing

Figure 29a: Clients can be positioned in the Pacer facing the rear (open end) of the frame. This is called posterior positioning. It allows advanced clients to move freely without obstructions below or in front of them.

Chest prompt (if used) opens front and back for posterior positioning and transfers.

1. **Apply the caster brakes** to immobilize the Pacer.
2. **Remove accessories.** Unfasten clamps around the top bars (see page 10).

3. **Turn accessories** to face open end of Pacer frame and reattach to the top bar.
4. **Reset swivel locks** in opposite direction if needed (see page 9).
5. **If any other prompts are required,** follow anterior positioning instructions in reverse (see Pages 27 and 28).
6. **Release caster brakes.**

For more details on accessories, function and recommended uses, go to:

Maintenance 🗝️

This product is designed and tested for an expected life of 5 years when used and maintained in accordance with this manual. At all times, clients must ensure that the product remains in a safe and useable condition, including regular maintenance and inspections as specified in this product manual.

To prevent structural failure, which may result in serious injury or death:

- Inspect this product and accessories regularly for loose or missing screws, metal fatigue, cracks, broken welds, missing attachments, general instability or other signs of excessive wear.
- Immediately remove this product from use when any condition develops that might make operation unsafe.
- Do not use Rifton components or products for any purpose other than their intended use.
- Replace or repair components or products that are damaged or appear to be unstable.
- Use only Rifton authorized replacement parts. Order information for replacement parts is provided on the back of this product manual.

Do not use petroleum-based or solvent-based lubricants on casters, but lubricate when necessary with silicone spray or graphite.

Cleaning 🧑 🏠 🗝️

As needed, clean with disinfectant wipes or a solution of up to 10% bleach. Do not use excessive amounts of water.

The straps with hook and loop closures may be laundered. Engage the closures before washing. Do not iron.

Wash casters with water after outdoor use. Avoid mud and sand.

Warranty Statement 🧑 🏠 🗝️

If a Rifton product breaks or fails in service during the first year, we will replace it free of charge.

Materials 🧰

- Steel hardware items (nuts, bolts, screws, etc) are typically zinc or nickel plated, or stainless steel.
- Upholstery items (pads, support blocks, padded prompts, etc) are typically polyurethane foam with a fire-retardant cover made from expanded vinyl.
- Frames are typically steel or aluminum tubing, welded together, and coated with a baked-on paint finish. Some frame components may also be stainless steel.
- Straps are typically made of polypropylene or nylon webbing.
- Plastic components are typically injection molded from a variety of industrial resins.

All components are lead free and not made with natural rubber latex.

User modifications 🧑🏠🧰

⚠️ WARNING To prevent serious injury or death, do not modify or alter Rifton products or components, or use Rifton products or components in conjunction with products from other manufacturers. Rifton does not accept responsibility for any modifications or alterations made to our components or products after they leave our premises. Customers modifying or altering our components or products, or using them in conjunction with products from other manufacturers, do so at their own risk.