

Shoulder P.A.D.— Pillow Abduction Device

Single Patient Use Only

Small 11640005
Medium 11640006
Large 11640007

IMPORTANT INFORMATION

Please read all instructions before use. Correct application is essential to proper functioning of product.

INDICATIONS






Soft tissue repairs, shoulder sprains and strains, S/P glenohumeral acromioplasty, surgical repair of rotator cuff, anterior glenohumeral capsular reconstruction, dislocation/subluxation of G-H joint.

PRECAUTIONS

- This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which they are responsible. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare practitioners, the patient, or other care providers involved in the patient's care.
- Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

INSTRUCTIONS FOR USE

1. Detach arm sling strap from front of arm sling. Place affected arm in sling so that it rests in the fold of the sling (1a). (Utilize thumb loop for additional comfort, if desired.) Secure front panel using outside o-ring (1b).
2. Bring arm sling strap across the back and opposite shoulder (2a) and pull through center o-ring to secure Velcro® back onto strap (2b). **Note:** Depending on right or left fitting, adjust Y-tab Velcro® strap ends so that the strap(s) secures back onto itself properly. Strap length may also be adjusted by removing Y-tab end, trimming the strap, and reapplying Y-tab end.
3. Align foam pillow at waistline on affected side with the wide end facing front (3a).

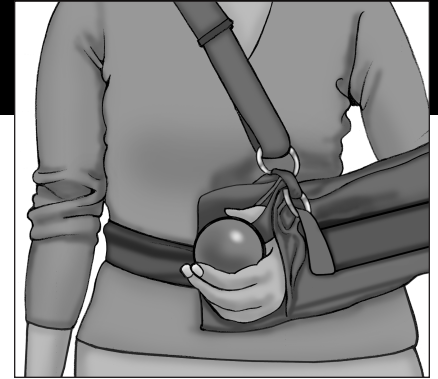

Shoulder P.A.D.— Pillow Abduction Device

Single Patient Use Only

Small 11640005
Medium 11640006
Large 11640007

IMPORTANT INFORMATION

Please read all instructions before use. Correct application is essential to proper functioning of product.

INDICATIONS





Soft tissue repairs, shoulder sprains and strains, S/P glenohumeral acromioplasty, surgical repair of rotator cuff, anterior glenohumeral capsular reconstruction, dislocation/subluxation of G-H joint.

PRECAUTIONS

- This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which they are responsible. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare practitioners, the patient, or other care providers involved in the patient's care.
- Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

INSTRUCTIONS FOR USE

1. Detach arm sling strap from front of arm sling. Place affected arm in sling so that it rests in the fold of the sling (1a). (Utilize thumb loop for additional comfort, if desired.) Secure front panel using outside o-ring (1b).
2. Bring arm sling strap across the back and opposite shoulder (2a) and pull through center o-ring to secure Velcro® back onto strap (2b). **Note:** Depending on right or left fitting, adjust Y-tab Velcro® strap ends so that the strap(s) secures back onto itself properly. Strap length may also be adjusted by removing Y-tab end, trimming the strap, and reapplying Y-tab end.
3. Align foam pillow at waistline on affected side with the wide end facing front (3a).







Attach arm sling to pillow by matching up hook and loop portions of Velcro® (3b).



4. Secure waist strap using o-rings on front and back end of the pillow (4a). Pull waist strap tightly before securing Y-tab Velcro® on each end (4b). The position of the pillow can be adjusted by sliding the pillow forward or back along the waistline to achieve the desired external or internal rotation. If cushion can be pushed downward with pressure, the waist strap needs to be tightened.



Part #0-1796
Revised 9/03
©2003 DeRoyal. All Rights Reserved.

CARE INSTRUCTIONS



Hand wash arm sling and pillow cover in luke warm water and air dry.



Attach arm sling to pillow by matching up hook and loop portions of Velcro® (3b).



4. Secure waist strap using o-rings on front and back end of the pillow (4a). Pull waist strap tightly before securing Y-tab Velcro® on each end (4b). The position of the pillow can be adjusted by sliding the pillow forward or back along the waistline to achieve the desired external or internal rotation. If cushion can be pushed downward with pressure, the waist strap needs to be tightened.



Part #0-1796
Revised 9/03
©2003 DeRoyal. All Rights Reserved.

CARE INSTRUCTIONS

Hand wash arm sling and pillow cover in luke warm water and air dry.