

How to Use Guide

Weelchair Customized

Placing the SitStand

PRIOR TO PLACING THE SITNSTAND, MAKE SURE THAT THE WHEELCHAIR BREAKS ARE LOCKED

A. Place the SitnStand folded on the wheelchair - Illustration A.

B. Insert the back part / Air Supply area between the back and the seat of the wheelchair -

Illustration B.

C. Place the air supply unit's slings on the wheelchair's handles and tighten them up -


Illustration C.


D. When not in use we recommend you attach the remote control to a velcro strip that will be attached to the wheelchair push handles -

Illustrations D1 + D2.









2


Sitting Down

LOCK THE WHEELCHAIR BRAKES BEFORE SITTING DOWN!

- A. Sit Comfortably in the center.
- B. Start deflating by pressing the **"Down"** arrow button.
- C. You Can Now Sit Down Comfortably.

**NOTE:

When using the battery for the first time it should be charged for at least 12 hours.



3

Standing Up

LOCK THE WHEELCHAIR BRAKES BEFORE SITTING DOWN!

- A. Take your feets off the wheelchair paddes and place them on the floor, close to the chair.
- B. Sit upright.
- C. Spread your feet.
- D. Inflate the cushion by pressing the "Up" button.
- E. Now you can easily Stand Up.
- **NOTE:

Incase of cognitive imperiment the SitnStand should only be oparated by a caregiver.




4

Get to Know the Remote Control

**NOTE:

Standby mode- flashes slowly (one flash/sec) | Working mode - flashes quickly (5 flashes/sec) | Malfunction reset - press the two control buttons simultaneously for 10 secs. If that doesn't help, please contact us at - info@sitnstand.com

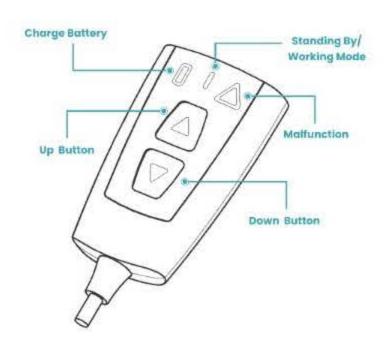

5

Standing Up

- A. Remove battery by sliding it towards you.
- B. Connect battery to the charger as illustrated.
- C. When the "Red" light on the charger changes to "Green", the battery is fully charged.
- D. Slide the charged battery into its place.

**NOTE:

When using the battery for the first time, it should be charged for at least 12 hours.

